

PI ORTHOPAEDIC

Sterile
Hydrogel Coating

SYNTHETIC
NOT MADE WITH
NATURAL RUBBER LATEX

The durability required for broaching and the tactility needed for pinning

- Thicker glove for **protection**¹
- Smooth finish for **tactile sensitivity**
- Water-based hydrogel coating for **easy donnability**
- Interlocking, beaded cuff design helps to **prevent roll-down**
- Proprietary hand mold with an independent thumb design allows for an **anatomical fit and natural movement**




Cardinal Health is dedicated to offering orthopaedic gloves that provide the protection wearers need so they can focus on providing the best outcomes for their patients.


Cardinal Health™ Protexis™ PI Orthopaedic Surgical Gloves are designed to provide the durable, quality protection orthopedic surgeons' need during tough surgical cases.

Properties (before aging)

Force at break	29N ⁶
Elongation at break (elasticity)	≥ 650% ²
Puncture resistance (cuff)	Min 5N ³
Freedom from holes	0.65 AQL ⁴
Sterilization	Gamma radiation
Accelerant	Zinc diethyldithiocarbamate (ZDBC), Zinc mercaptobenzothiazole (ZMBT), Diphenylguanidine (DPG)

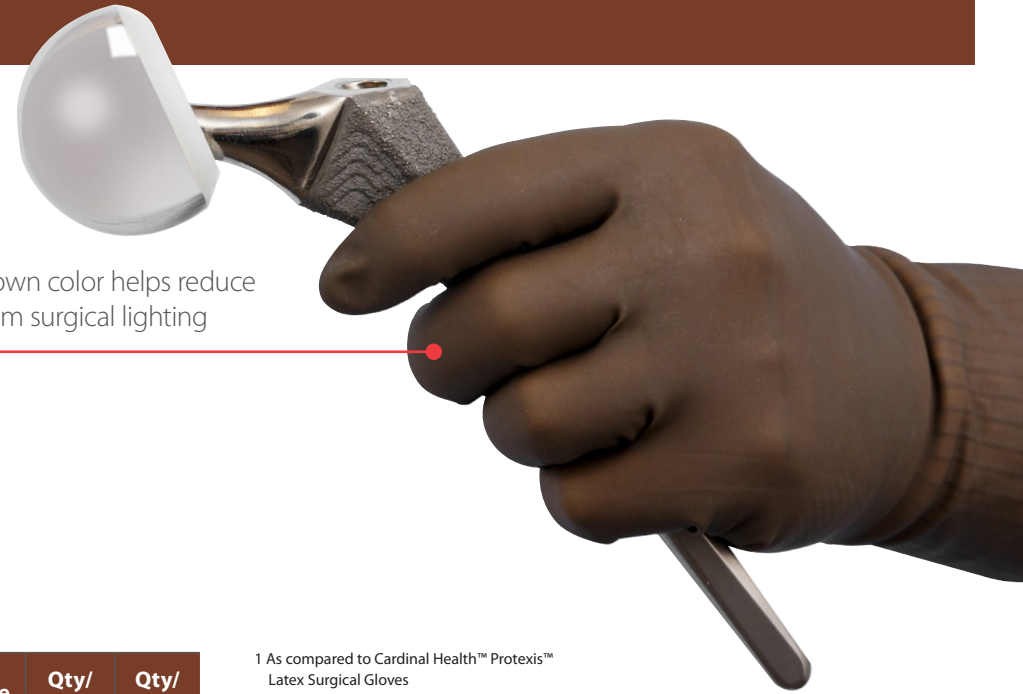

Rich, brown color helps reduce glare from surgical lighting

Catalog no.	Size	Length	Thickness ²			Material	Color	Cuff type	Qty/ bx	Qty/ cs
			Finger	Palm	Cuff					
2D73HT60	6	291mm	0.34mm	0.26mm	0.21mm	Synthetic polyisoprene (PI) with water-based hydrogel polymer coating		Beaded/ Rolled	40	160
2D73HT65	6.5									
2D73HT70	7									
2D73HT75	7.5									
2D73HT80	8									
2D73HT85	8.5									
2D73HT90	9									

- 1 As compared to Cardinal Health™ Protexis™ Latex Surgical Gloves
- 2 In accordance with ASTM D 3577
- 3 Tested in accordance with AS/NZS 4179, average test result = 7N (before aging)
- 4 Tested in accordance with EN 455-1
- 5 35% reduction of materials used as compared to previous Cardinal Health packaging design.
- 6 Tested in accordance with EN455-2

THE CARDINAL HEALTH™ PROTEXIS™ SURGICAL GLOVES PROMISE:

We protect so you can perform.

Cardinal Health is dedicated to providing protection, performance and expertise so wearers can perform confidently and focus on their patients.



Help maximize storage space: Half-fold packaging design reduces packaging material.⁵



Store recommendation: Do not store near sources of ultraviolet light, heat or x-rays. Store in a cool, dry place, store away from direct sunlight.



Expiration: 35 months from date of manufacture. Expiration date is printed on packaging.

For healthcare professionals only

Important information: Prior to use, refer to the instructions on the dispenser box supplied with this device for indications, contraindications, side effects, suggested procedure, warnings and precautions.

As part of its continuous product development policy, Cardinal Health reserves the right to change product specifications without prior notification

Please contact your Cardinal Health representative for additional product availability information.

